

Siège social:

Avenue de la Libération  
42720 BRIENNON - FRANCE  
Tél : +33 (0)4 77 60 79 99  
Fax : +33 (0)4 77 60 79 90

At Briennon the 18 of July, 2023

From Laure OLIVER/PRRC


oliver@evolutis42.com

Our old recommendations were originally the 132/4min cycle and All countries was already following its own recommendations. I confirm that the Cycle 134°C/18min is a cycle following a French cycle "the prion cycle". We wanted to standardize our France-Export practices.

The hospitals can used their internal procedure in condition that the cycle used was validated, the recommendations in the IFU are regulatory and allow you to inform hospitals if they do not have a validated cycle.

**We realized a second validation test for the cycle 134°C/4min and we can confirm the conformity of this cycle with our instruments so you can use this cycle.**

Best regards

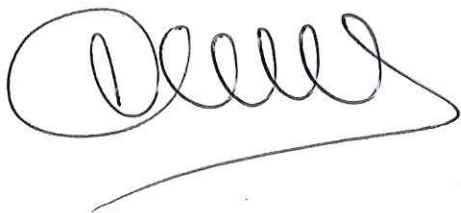

**EVOLUTIS SAS**

SAS au capital social de 1 043 320 euros  
10 place des TUILIERS  
42720 BRIENNON  
Tél. 04 77 60 79 99 - Fax 04 77 60 79 90  
RCS ROANNE 423 551 047 00013 APE 3200 A